

Catalog Number

TBS42030-100

TBS42030-200

Kit Size

100 assays

200 assays

DESCRIPTION

Mycoplasma Species qPCR Kit has been designed to specifically identify the mycoplasma genus species in a single PCR reaction using real-time quantitative polymerase chain reaction (qPCR) and probe fluorescence labels. The detection of the target DNA confirms ingredient authenticity and prevents food fraud, ethical issues, or health concerns. Tribioscience's Mycoplasma qPCR is very sensitive, accurate, and High efficiency (See Fig.1, and Table 1).

PRINCIPLE

Authenticating ingredients utilizes real-time PCR which is based on the amplification of a specific region of the relevant target genome. The amplified product is detected using target-specific fluorescent probes that bind to the amplified product. As the PCR product accumulates, there is an increased fluorescent signal from the bound probes. Monitoring the fluorescence intensities during the PCR run allows the detection of the accumulating PCR product in real time.

Tribioscience's Mycoplasma qPCR Kit includes mycoplasma positive and negative controls, PCR internal controls labeled with Hex, a qPCR super mix, and the primer-probe mix in which the probe has been labeled with FAM for the target gene. These aid in a straightforward interpretation of the results.

KEY FEATURES

- ❖ High sensitivity and specificity for mycoplasma species.
- ❖ High efficiency: the optimal systemic conditions for PCR amplifications.
- ❖ Streamlined protocol: Just add DNA Template and water.
- ❖ No cross reactivity with other species.

APPLICATIONS

Detect mycoplasma-target DNA in contaminated cell cultures, FBS medium, plant, cannabis, cannabis ingredients, grain, food, herbals, and animal feed.

KIT CONTENTS

Name	100x rxn	200x rxn
Myco qPCR Mix	0.8mL	1.6mL
Myco Primer-probe Mix	0.6mL	1.2mL
Myco Positive Control DNA	50μL	100μL
Negative Control	50μL	100μL
Nuclease Free Water	1mL	2x 1mL

The mycoplasma target probe has been labeled with **FAM** while the PCR internal control has been labeled with **Hex**.

STORAGE CONDITION

The kit is shipped on ice and stored at -20°C for long-term storage. Shelf life of 12 months after receipt.

SAMPLE DNA PREPARATION

Three sample DNA preparation methods are recommended as below. These methods are validated with cultured mycoplasma medium. The typical data is shown in the fig. 3.

Note: we recommend client to optimize a suitable method for a specific sample.

Method A: Boiling Sample

Add 200μL of the Mycoplasma Cell Culture into a 1.5 mL screw capped microtube and place it into the boiling water for 7min. Afterwards, spin it at 13000rpm for 1min. The supernatant can be used as DNA for qPCR amplification or stored at -20°C for further use.

Method B: Enrichment plus Boiling

Add 1mL of the Mycoplasma Cell Culture into a 1.5 mL screw capped microtube. Then, spin it at 13000rpm for 10min to sediment the mycoplasma particles. After then, pour out the supernatant into the waste and resuspend the pellets in 50μL 1x TE buffer. Boiling it for 10min. Spin it at 13000rpm for 1min. This is the enriched DNA sample for qPCR amplification or stored at -20°C for further use.

Method C: Simple DNA Extraction (Enrichment + Extraction)

The sediment of the mycoplasma particles is as same as Method B. Afterwards, pour out the supernatant, and add 40μL of Fast DNA extract (TBS6008), incubate at 67°C in the water bath for 15min. Then add 160μL of DEPC water and boiling for 10min. This is the extracted DNA sample for qPCR amplification or stored at -20°C for further use.

PCR PROTOCOL

1. Set up PCR reaction for each sample in 20μL

Reaction Component	Volume (μL)
qPCR Super Mix	7.0
Primer-probe Mix	5.0
Nuclease-free Water	3.0
DNA sample	5.0
Final Volume	20μL

The Positive Control (5μL DNA/reaction) and Negative Control (5μL DNA/reaction) should be included in PCR Test. In addition, Positive control can be used for Standard curve as 10x sequentially dilution. The Copy number is labeled in the vial.

2. Suggested PCR conditions

Step	Amplification	PCR	
		CYCLE (40x cycles)	
	HOLD	Denature	Anneal/ Extend
Temperature	95°C	95°C	60°C
Time	2 min	15 sec	30 sec

DATA ANALYSIS

Positive Reaction: Sample Ct ≤ 37 w/ Positive, Negative and Blank controls normal.

Negative Reaction: Sample Ct ≥ 38 w/ Positive, Negative and Blank controls normal.

PCR internal control is positive in all samples, positive and negative controls. The positive response indicates a normal PCR amplification. Otherwise, the PCR reaction may be inhibited.

Repeat Reaction: If one of the control reactions is not normal, PCR reaction is failed, and should be repeated.

Fig.1. Mycoplasma DNA concentration dependent qPCR Amplification (FAM)

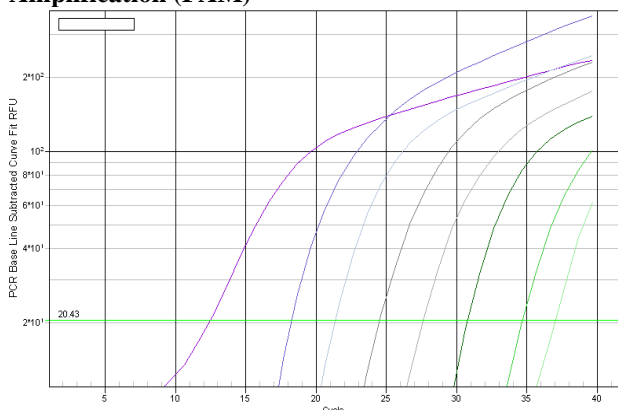


Fig.2 Internal Control Gene qPCR Amplification (Hex)

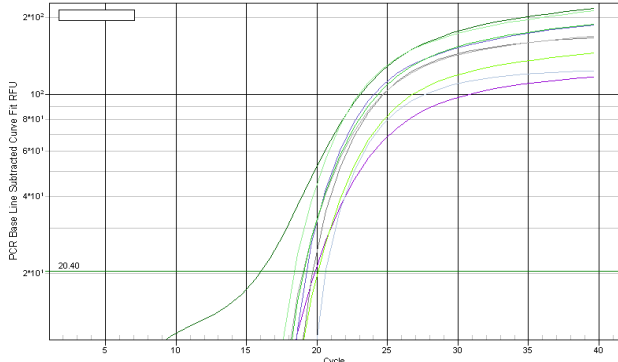


Table 1: Mycoplasma DNA qPCR Sensitivity

MycDNA test (GC/ml)	Threshold Cycle
10^8	12.45
10^7	18.2
10^6	21.32
10^5	24.48
10^4	27.59
10^3	30.76
10^2	34.66
10^1	36.95
Negative Control	N/A

Fig.3. Mycoplasma DNA preparation method validation

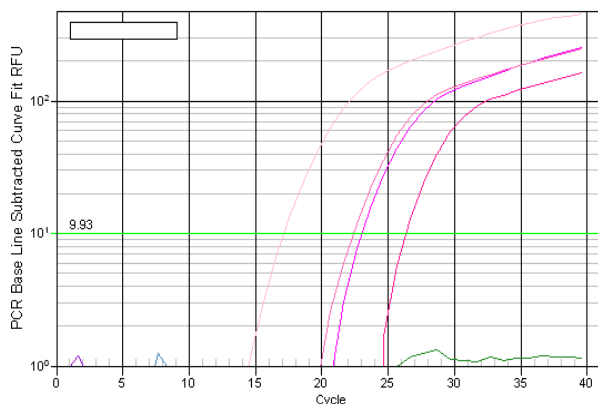


Table 2: Mycoplasma DNA efficiency comparison from 3 methods

Mycoplasma DNA	Threshold Cycle (Ct)
Method A: Boiling	26.44
Method B: Enrichment	23.11
Method C: Simple DNA extraction	22.50
Positive	17.24
Negative	N/A

RELATIVE PRODUCTS

TBS6025: Microbial DNA Magnetic Extraction
TBS42020: Universal Aspergillus qPCR
TBS42021: Aspergillus Flavus qPCR
TBS42022: Aspergillus Fumigatus qPCR
TBS42023: Aspergillus Niger qPCR
TBS42024: Aspergillus Terreus qPCR
TBS42025: 4-In-1 Aspergillus qPCR
TBS42026: O157H7 E. Coli qPCR
TBS42027: STEC qPCR
TBS42028: Salmonella qPCR
TBS42029: STEC and Salmonella Multiple qPCR
TBS42031: Listeria Monocytogenes qPCR
TBS42033: Bacillus Cereus qPCR
TBS42033: Bacillus Species qPCR

For research use only.