

For the quantitative determination of human VEGF concentrations in cell culture supernates, serum, and plasma.

**INTRODUCTION**


Vascular endothelial growth factor (VEGF) is also known as vascular permeability factor (VPF). In humans, VEGF expresses alternatively spliced isoforms of amino acids 121, 145, 165, 183, 189 and 206 in length. VEGF is expressed in a variety of cells and tissues, including skeletal and cardiac muscle, hepatocytes, osteoblasts, neutrophils, macrophages, keratinocytes, brown adipose tissue, CD34+ stem cells, endothelial cells, fibroblasts, and vascular smooth muscle cells. In addition, VEGF is a potent mediator of fetal angiogenesis and vasculogenesis, and during embryogenesis, VEGF regulates the proliferation, migration, and survival of endothelial cells, thereby regulating blood vessel density and size. Moreover, VEGF levels correlate with disease activity in autoimmune diseases such as rheumatoid arthritis, multiple sclerosis, and systemic lupus erythematosus.

The Tribo™ Fast Human VEGF ELISA is designed to quantitatively detect Human VEGF levels in different tissues including skin, muscle, neural, serum, and other biological samples. The main feature is that **the kit uses our novel proprietary approaches to combine samples and detections into a one-step instead of the complicated traditional methods.** It makes the assay simple, easy, accurate and fast. The measurement can be finished in 3 hours, with no need for 4-5 hours (Fig. 1). The detection range is from 15 to 1000 pg/mL. The levels of human VEGF samples are parallel to the standard curves obtained using the kit standards linearly. These results indicate that this kit can be used to determine relative mass values for natural human VEGF protein.

**PRINCIPLE OF THE ASSAY**

This assay employs the quantitative sandwich enzyme immunoassay technique (See Fig. 1). A monoclonal antibody specific for human VEGF was pre-coated onto a microplate. Standards and samples are pipetted into the wells, and then incubated with HRP-conjugated detection antibody specific for human VEGF. Following a wash to remove any unbound antibody and samples, an **ultra-sensitive TMB substrate solution** is added to the wells for color development. The color intensity is in proportion to the amount of VEGF bound in the initial step. The intensity of the color is measured by plate read at 450 nm.

**Fig. 1: Assay Principle:**

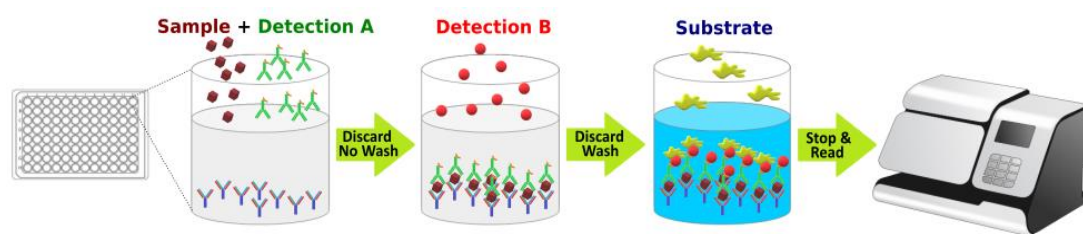

**KIT CONTENT AND STORAGE CONDITIONS**

PART	PART#	DESCRIPTION	STORAGE OF OPENED/ RECONSTITUTED
Human VEGF Microplate	TBS3264A	96 well polystyrene microplate (12 strips of 8 wells) coated with a polyclonal antibody specific for human VEGF.	Return unused wells to the foil pouch. Reseal along the entire edge of the zip-seal. May be stored for up to 1 month at 2-8 °C.
Human VEGF Standard	TBS3264B	30 µl of Recombinant human VEGF protein (50ng/mL).	Aliquot and store at -20 °C for up to 1 month in a manual defrost freezer. Avoid repeated freeze-thaw cycles.
Detection A	TBS3264C	2.1 ml of Biotin-Human VEGF antibody.	May be stored for up to 3 months at 2-8 °C.*
Detection B	TBS3264D	300 µl of Streptavidin-HRP.	
Assay Diluent	TBS3264E	25 ml of a buffered protein base with preservatives.	
Wash Buffer	TBS3000W	12 ml of concentrated solution (10x).	
TMB Substrate	TBS3000T	12 ml of ultra-sensitive TMB substrate.	
Stop Solution	TBS3000S	6ml of 2 N sulfuric acid.	

Store the unopened kit at 2-8°C. Do not use past kit expiration date.

The kit contains sufficient materials to run an ELISA on one 96 well plate.

**PRECAUTIONS**

Wear protective gloves, clothing, eye, and face protection. Wash hands thoroughly after handling.

**REAGENT PREPARATION**

**Bring all reagents to room temperature before use.**

**Wash Buffer:** Add 12 mL of Wash Buffer Concentrate (10x) to 108 mL of deionized distilled water to prepare 120 mL of Wash Buffer (*If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved.*).


**Detection B working solution preparation:** Add 240 µL of **Detection B** streptavidin-HRP to 12 mL Assay Diluent to prepare Detection B working solution.

**Human VEGF Standard Preparation:**

Label test tubes as #1 through #8. Pipet 490 µL of 1x Assay Diluent into tube #1, and 250 µL into tubes #2 to #7 as diagram below (Fig.2).

1. Add 10 µL of the Human VEGF Standard stock solution (50ng/mL) by dilution of 50X to tube #1 (1000pg/mL), and mix.
2. Make 2x serial dilutions of the standard using the 250pg/mL standard solution (tube #1) from tube #2 through #7 with sequential transfer of 250 µL to the next concentration. Mix each tube thoroughly before the next transfer. The standard concentration in tube 1 through 7 will be 1000, 500, 250, 125, 62.5, 31.3, and 15.6 pg/mL. Tube# 8 is Standard 0.

**Fig.2 Diagram for Human VEGF standard preparation**

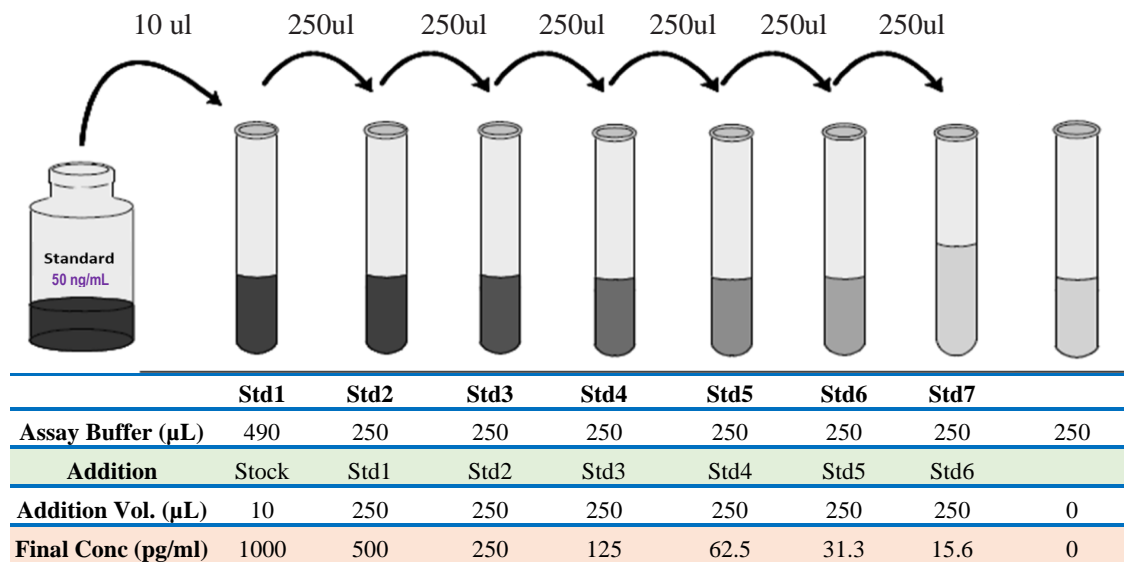

**ASSAY PROCEDURE**

**Bring all reagents and samples to room temperature before use. It is recommended that all standards, controls, and samples be assayed in duplicate.**

1. Add 80 µL of standard, sample, or control per well.
2. Add 20 µL of **Detection A** to the above standard and sample of each well, thoroughly mix. Cover with the adhesive sealer. Incubate at **RT for 2 hours**.
3. Aspirate each well (no wash). Invert the plate and blot it against clean paper towels.
4. Add 100 µL of **Detection B** to each well. Incubate at **RT for 1 hour**.
5. Aspirate each well, and wash for 3 times by filling each well with 200 µL Wash Buffer (*Complete removal of liquid at each step is essential to good performance*). After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.

6. Add 100 µL of **TMB Substrate** to each well. Incubate **at RT for 10-20 min** (*Protect from light*). The color becomes blue.
7. Add 50 µL of **Stop Solution** to each well. The color in the well should change from blue to yellow (gently tap the plate to ensure thorough mixing).
8. Determine the optical density of each well within 20 minutes, using a microplate reader at 450 nm. If wavelength correction is available, set to 540 nm or 570 nm. If wavelength correction is not available, subtract readings at 540 nm or 570 nm from the readings at 450 nm. This subtraction will correct for optical imperfections in the plate. Readings made directly at 450 nm without correction may be higher and less accurate.

**CALCULATION OF RESULTS**

Average the duplicate readings for each standard, control, and sample subtract the average zero standard optical density (O.D.).

Create a standard curve using computer software capable of generating a four parameter logistic (4-PL) curve-fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the Y-axis against the concentration on the X-axis and draw a best fit curve through the points on the graph. The data may be linearized by plotting the log of the human VEGF concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data.

**TYPICAL DATA**

This standard curve ( $R^2=0.9995$ ) is provided for demonstration only. A standard curve should be generated for each set of samples assayed. Fig. 3 is an example of typical Data.

**SENSITIVITY**


The minimum detectable dose (MOD) of human VEGF is typically 10 pg/ml.  
The Intra-assay CV is 3.79% the Inter-assay CV is <10%.

**SPECIFICITY**

This assay recognizes natural and recombinant human VEGF.

**RELATIVE PRODUCTS**

- Human IL-1β ELISA (TBS3219)
- Human IL-2 ELISA (TBS3220)
- Human IL-4 ELISA (TBS3221)
- Human IL-6 ELISA (TBS3223)
- Human IL-7 ELISA (TBS3224)
- Human IL-8 ELISA (TBS3225)
- Human IL-10 ELISA (TBS3226)
- Human IL-13 ELISA (TBS3227)
- Human IL-17 ELISA (TBS3228)
- Human IL-22 ELISA (TBS3229)
- Human IFN-gamma ELISA (TBS3230)
- Human TGF- β1 ELISA (TBS3232)
- Human GM-CSF ELISA (TBS3233)
- Human MIP-1α ELISA (TBS3234)

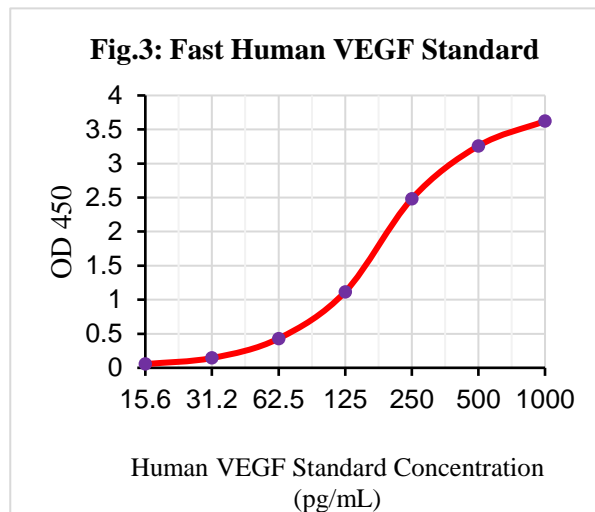

**For research use only.**