

For the quantitative determination of rat IL-1 $\beta$  concentrations in cell culture supernatants, serum, and plasma.

**INTRODUCTION**

Interleukin-1 beta (IL-1 $\beta$ ) is a potent pro-inflammatory cytokine produced primarily by activated monocytes, macrophages, and dendritic cells in response to infection or cellular damage. IL-1 $\beta$  plays a central role in initiating and amplifying inflammatory responses, including inducing fever, promoting immune cell recruitment, and stimulating the production of other cytokines. While essential for host defense, dysregulated IL-1 $\beta$  activity is implicated in various inflammatory and autoimmune diseases, such as rheumatoid arthritis, type 2 diabetes, and multiple sclerosis.

The Tribioscience Rat IL-1 $\beta$  ELISA is designed to quantitatively detect rat IL-1 $\beta$  levels in different tissues including skin, muscle, neural, serum, and other biological samples. The main feature is that **the kit uses our novel proprietary approaches to combine samples and detections into a one-step instead of the complicated traditional methods. It makes the assay simple, easy, accurate and fast. The measurement can be finished in 3 hours, not need 4-5 hours (Fig. 1). The detection range is from 62 to 4000 pg/mL.** The levels of rat IL-1 $\beta$  samples are parallel to the standard curves obtained using the kit standards linearly. These results indicate that this kit can be used to determine relative mass values for natural rat IL-1 $\beta$  protein.

Alternative names: Interleukin-1 beta; IL-1 beta; IL-1 $\beta$ ; Interleukin-1 $\beta$ ; IL-1b

**PRINCIPLE OF THE ASSAY**

This assay employs the quantitative sandwich enzyme immunoassay technique (See Fig. 1). A monoclonal antibody specific for rat IL-1 $\beta$  was pre-coated onto a microplate. Standards and samples are pipetted into the wells, and then, incubated with HRP-conjugated detection antibody specific for rat IL-1 $\beta$ . Following a wash to remove any unbound antibody and samples, an **ultra-sensitive TMB substrate solution** is added to the wells for color development. The color intensity is in proportion to the amount of IL-1 $\beta$  bound in the initial step. The intensity of the color is measured by plate read at 450 nm.

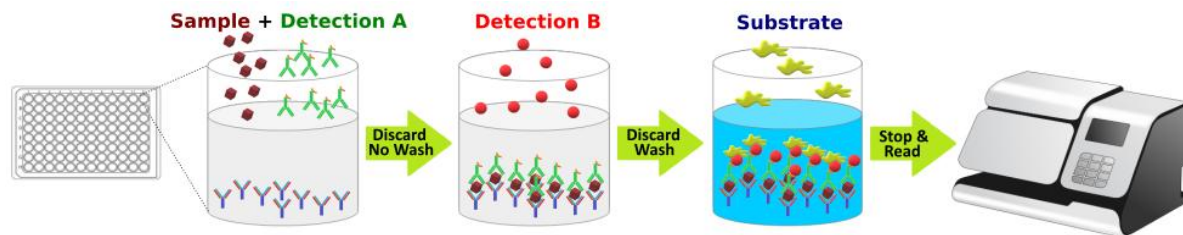


Fig.1: Simple ELISA procedure

**KIT CONTENT AND STORAGE CONDITIONS**

PART	PART#	DESCRIPTION	STORAGE OF OPENED/ RECONSTITUTED
Rat IL-1 $\beta$ Microplate	TBS3055A	96 well polystyrene microplate (12 strips of 8 wells) coated with a polyclonal antibody specific for rat IL-1 $\beta$ .	Return unused wells to the foil pouch. Reseal along the entire edge of the zip-seal. May be stored for up to 1 month at 2-8 °C.
Rat IL-1 $\beta$ Standard	TBS3055B	20 $\mu$ l of Recombinant rat IL-1 $\beta$ protein (200 ng/mL).	Aliquot and store at -20 °C for up to 1 month in a manual defrost the freezer. Avoid repeated freeze-thaw cycles.
Detection A	TBS3055C	2.1 ml of Biotin-Rat IL-1 $\beta$ antibody.	May be stored for up to 3 months at 2-8 °C.
Detection B	TBS3055D	200 $\mu$ L of Streptavidin-HRP.	
Assay Diluent	TBS3055E	25 ml of a buffered protein base with preservatives.	
Wash Buffer	TBS3000W	12ml of concentrated solution(10x).	
TMB Substrate	TBS3000T	12 ml of ultra-sensitive TMB substrate.	
Stop Solution	TBS3000S	6ml of 2 N sulfuric acid.	

Store the unopened kit at 2-8 °C. Do not use past kit expiration date.  
The kit contains sufficient materials to run an ELISA on one 96 well plate.

**PRECAUTIONS**

Wear protective gloves, clothing, eyes, and face protection. Wash hands thoroughly after handling.

**REAGENT PREPARATION**

**Bring all the reagents to room temperature before use.**

**Wash Buffer:** Add 12 mL of Wash Buffer Concentrate (10x) to 108 mL of deionized distilled water to prepare 120 mL of Wash Buffer (*If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved*).


**Detection B working solution preparation:** Add 150  $\mu$ L of **Detection B** streptavidin-HRP to 12 mL Assay Diluent (TBS3055E) to prepare Detection B working solution.

**Rat IL-1 $\beta$  Standard Preparation:**

Label test tubes as #1 through #8. Pipet 490  $\mu$ L of 1x Assay Diluent into tube #1, and 250  $\mu$ L into tubes #2 to #8 as diagram below.

1. Add 10  $\mu$ L of the Rat IL-1 $\beta$  Standard stock solution (200 ng/mL) by dilution of 50X to tube #1 and mix.
2. Make 2x serial dilutions of the standard using the 4000 pg/mL standard solution from tube #2 through #7 with sequential transfer of 250  $\mu$ L to the next concentration. Mix each tube thoroughly before the next transfer. The standard concentration in tube 1 through 7 will be 4000, 2000, 1000, 500, 250, 125 and 62.5 pg/mL. Tube# 8 is Standard 0.

**Fig.2 Diagram for Rat IL-1 $\beta$  standard preparation**

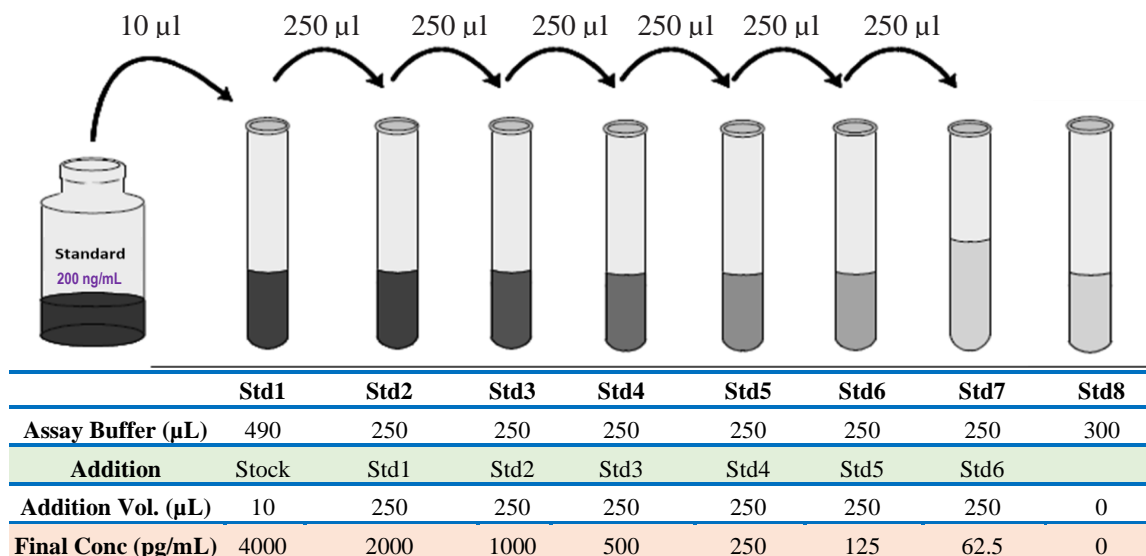

**ASSAY PROCEDURE**

**Bring all reagents and samples to room temperature before use. It is recommended that all standards, controls, and samples be assayed in duplicate.**

1. Add 80  $\mu$ L of standard, sample, or control per well.
2. Add 20  $\mu$ L of **Detection A** to the above standard and sample of each well, thoroughly mix. Cover with the adhesive sealer. Incubate at **RT for 2 hours**.
3. Aspirate each well (no wash). Invert the plate and blot it against clean paper towels.
4. Add 100  $\mu$ L of **Detection B** to each well. Incubate at **RT for 1 hour**.
5. Aspirate each well, and wash for 3 times by filling each well with 300  $\mu$ L Wash Buffer (*Complete removal of liquid at each step is essential to good performance*). After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
6. Add 100  $\mu$ L of **TMB Substrate** to each well. Incubate **at RT for 10-20min** (*Protect from light*). The color becomes blue.
7. Add 50  $\mu$ L of **Stop Solution** to each well. The color in the well should change from blue to yellow (gently tap the plate to ensure thorough mixing).
8. Determine the optical density of each well within 20 minutes, using a microplate reader at 450 nm. If wavelength

correction is available, set to 540 nm or 570 nm. If wavelength correction is not available, subtract readings at 540 nm or 570 nm from the readings at 450 nm. This subtraction will correct for optical imperfections in the plate. Readings made directly at 450 nm without correction may be higher and less accurate.

**CALCULATION OF RESULTS**

Average the duplicate readings for each standard, control, and sample subtract the average zero standard optical density (O.D.).

Create a standard curve using computer software capable of generating a four parameter logistic (4-PL) curve-fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the Y-axis against the concentration on the X-axis and draw a best fit curve through the points on the graph. The data may be linearized by plotting the log of the rat IL-1 $\beta$  concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data.

**TYPICAL DATA**

This standard curve ( $R^2=1.000$ ) is provided for demonstration only. A standard curve should be generated for each set of samples assayed. Fig. 3 is an example of typical Data.

**SENSITIVITY**


The minimum detectable dose (MDD) of Rat IL-1 $\beta$  is typically 62 pg/ml.  
The Intra-assay CV is < 10% the Inter-assay CV is < 12%.

**SPECIFICITY**

This assay recognizes natural and recombinant rat IL-1 $\beta$ .  
No cross-reactivity with others.

**RELATIVE PRODUCTS**

- Mouse IL-1 $\beta$  ELISA (TBS3219)
- Mouse IL-2 ELISA (TBS3220)
- Mouse IL-4 ELISA (TBS3221)
- Mouse IL-6 ELISA (TBS3223)
- Mouse IL-7 ELISA (TBS3224)
- Mouse IL-8 ELISA (TBS3225)
- Mouse IL-10 ELISA (TBS3226)
- Mouse IL-13 ELISA (TBS3227)
- Mouse IL-17 ELISA (TBS3228)
- Mouse IL-22 ELISA (TBS3229)
- Mouse IFN-gamma ELISA (TBS3230)
- Mouse TGF-  $\beta$ 1 ELISA (TBS3232)
- Mouse GM-CSF ELISA (TBS3233)
- Mouse MIP-1 $\alpha$  ELISA (TBS3234)
- Rat TNF-alpha ELISA (TBS3054)

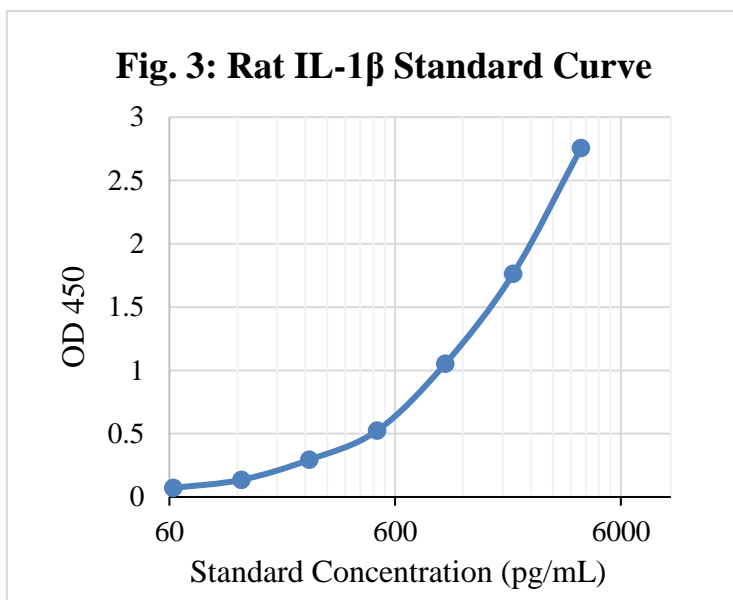

**For research use only. Not for use in diagnostic procedures.**